



GIMA

PROFESSIONAL MEDICAL PRODUCTS

GIMACARE

3-in-1 Combo Electrotherapy

Use and maintenance book

GIMA 28406



Shenzhen Roundwhale Technology Co., Ltd.
202, 2/F, Building 27, Dafa Industrial Park, Longxi
Community, Longgang District, Shenzhen, China.
E-mail: info@roovjoy.com
MADE IN CHINA



R-C1



2460



Shanghai International Holding Corp. GmbH(Europe)
Eiffestrasse 80, 20537 Hamburg, Germany
shholding@hotmail.com



Gima S.p.A.

Via Marconi, 1 - 20060 Gessate (MI) Italy
gima@gimaitaly.com - export@gimaitaly.com

www.gimaitaly.com

INSTRUCTION MANUAL
FOR
3-in-1 Combo Electrotherapy Device
Model: R-C1



Shenzhen Roundwhale Technology Co., Ltd.
This manual is valid for the R-C1 Stimulator

Be sure to read this instruction manual before operate and
keep it where safe.

This user manual is published by Shenzhen Roundwhale
Technology Co., LTD.

Shenzhen Roundwhale Technology Co., Ltd. does not guarantee its contents and reserves the right to improve and amend it at any time without prior notice. However, Amendments will be published in a new edition of this manual.

All Rights Reserved.

R-C1 Rev.V1.0© 2025, printed in Nov. 10, 2025.

Declaration of conformity:

Shenzhen Roundwhale Technology Co., Ltd. declares that the device complies with following normative documents: IEC60601-1, IEC60601-1-2, IEC60601-1-11, IEC60601-2-10, IEC62304, ISO10993-5, ISO10993-10, ISO10993-1, ISO10993-23, ISO14971

TABLE OF CONTENTS

1. FOREWORD	5
2. SAFETY INFORMATION	7
3. GETTING TO KNOW YOUR DEVICE	13
4. SPECIFICATION	15
5. OPERATING INSTRUCTION	17
6. INSTRUCTIONS FOR USE	22
7. PROGRAM	30
8. CLEANING AND MAINTENANCE	32
9. TROUBLESHOOTING	33
10. STORAGE	35
11. DISPOSAL	36
12. ELECTROMAGNETIC COMPATIBILITY (EMC) TABLES	36
13. NORMALIZED SYMBOLS	42
14. WARRANTY	43

1. FOREWORD

Introduction

The device is a dual channel output TENS, EMS and MASSAGE stimulator. Before using, please read all the instructions in this user manual carefully and keep it safe for future use.

The stimulator belongs to the group of electrical stimulation systems. It has three basic functions – TENS (Transcutaneous Electrical Nerve Stimulation) , EMS (Electronic Muscle Stimulation) and MASSAGE.

Function of the stimulator: The device has 36 programs (18 TENS programs, 15 EMS programs and 3 MASSAGE programs) and applies electric currents in the low-frequency range for therapy. Each program controls the generated electric impulses, their intensity, frequency and pulse width. The parameters for each program are listed in clause 7.1.

Based on simulating the body's natural pulses, the mechanism of electrical stimulation equipment is to create electric impulses that are transcutaneous transmitted to nerves or muscle fibers through electrode . The intensity of the dual channel can be adjusted independently and can be applied individually to one body part. This dual channel device can be used with four pieces of electrodes, which allows you to stimulate one muscle groups simultaneously with a wide selection of standard programs. The electrical pulse is firstly transmitted to the tissue, then it affects the transmission of stimulation in nerves as well as muscle tissues in the body parts.

1.2 Medical background

1.2.1 ABOUT PAIN

Pain is an important signal in the human body warning system. It reminds us that something is wrong, without which, abnormal conditions may go undetected, causing damage or injury to vital parts of our bodies. Even though pain is a necessary warning signal of trauma or malfunction in the body, nature may have gone too far in its design.

Aside from its function in diagnosis, long-lasting persistent pain serves useless purpose.

Pain does not occur until encoded message travels to the brain where it is decoded, analyzed, and reacted to, from the injured area along the small nerves leading to the spinal cord. There the message is transmitted to different nerves that travel up the spinal cord to the brain. Then the pain message is interpreted, referred to and pain is felt.

1.2.2 WHAT IS TENS ?

TENS (Transcutaneous Electrical Nerve Stimulation) is effective in relief of pain. It is daily used and clinically proven by physiotherapists, caregivers and top athletes around the world. High-frequency TENS currents activates the pain-inhibiting mechanisms of the nervous system. Electrical impulses from electrodes, placed on the skin over or near the pain area, stimulate the nerves to block the pain signals to the brain, causing the pain go unperceived. Low-frequency TENS currents facilitate the release of endorphins, the body's natural painkillers.

1.2.3 WHAT IS EMS ?

Electrical Muscle Stimulation is an internationally accepted

and proven way of treating muscular injuries. It works by sending electronic pulses to the muscle needing treatment. That causes the muscle to exercise passively. It is a product deriving from the square waveform, originally invented by John Faraday in 1831. Through the square wave pattern it is able to work directly on muscle motor neurons. The EMS System has low frequency and this in conjunction with the square wave pattern allows direct work on muscle groupings.

2. SAFETY INFORMATION

2.1 Intended use

Intended purpose

The device is designed to be used for temporary relief of pain, including the acute and chronic pain relief.

The device is designed to be used for stimulate muscles for prevention of muscular atrophy, muscle strengthening and improve, Increasing local blood circulation and facilitate muscle performance.

Target population

The device using the object (patient) must be 18 years or older of adults.

Intended user

Medical staff or lay persons.

Intended condition

Intended for use in the home, hospital and health care facilities.

Indications

1) It is used for temporary relief of pain associated with sore and aching muscles in the neck, shoulder, back, joint, hip, hand, abdomen, upper extremities (arm) and lower extremities (leg) due to strain from exercise or normal household work activities.

2) Relaxation of muscle spasms.

3) Prevention or retardation of disuse atrophy.

- 4) Increasing local blood circulation.
- 5) Muscle re-education.
- 6) Immediate post-surgical stimulation of calf muscles to prevent venous thrombosis.
- 7) Maintaining or increasing range of motion.

2.2 Important Safety Precautions and Warnings



It is important that you read all the warnings and precautions included in this manual because they are intended to keep you safe, prevent risk of injury and avoid a situation that could result in damage to the device.

SAFETY SYMBOLS USED IN THIS MANUAL

2.2.1 Contraindication

- 1) Do not use this device if you have a cardiac pacemaker, implanted defibrillator, or other implanted metallic or electronic device. Such use could cause electric shock, burns, electrical interference, or death. 
- 2) The device should not be used when cancerous lesions or other lesions are present in the treatment area.
- 3) Stimulation should not be applied over open wounds or rashes, or over swollen, red, infected, or inflamed areas or skin eruptions (e.g. phlebitis, thrombophlebitis, varicose veins, arteriosclerosis obliterans etc.).
- 4) Electrode placements must be avoided that apply current to the carotid sinus region (anterior neck) or transcranially (through the head).
- 5) Apprehensive patients-usage of Electrical stimulation requires patient cooperation, hence the procedure shouldn't be attempted in patients with a communication handicap or a mental disability.  
- 6) Patients with cerebrovascular problems-patients with a history of aneurysm, stroke and transient ischaemia

shouldn't be treated using electrical stimulation, as it stimulates peripheral blood flow which can be fatal in such cases.

- 7) Epileptic patients-Electrical stimulation "pulses" have the potential to trigger a seizure.
- 8) Acute pain cases/pain of unknown etiology-usage of TENS in undiagnosed cases may hinder in the diagnosis.
- 9) Do not use in pregnancy, especially in the first trimester.

2.2.2 WARNING

- 1) If you have had medical or physical treatment for your pain, consult with your physician before use.
- 2) If your pain is not subdued, becomes more than mild, or lasts for more than five days, stop using the device and consult with your physician.
- 3) Do not apply stimulation over your neck because this could cause severe muscle spasms resulting in closure of your airway, difficulty in breathing, or adverse effects on heart rhythm or blood pressure.
- 4) Do not apply stimulation across your chest because the introduction of electrical current into the chest may cause rhythm disturbances to your heart, which could be lethal.
- 5) Do not apply stimulation over, or in proximity to, cancerous lesions.
- 6) Do not apply stimulation in the presence of electronic monitoring equipment (e.g., cardiac monitors, ECG alarms), which may not operate properly when electrical stimulation device is in use.
- 7) Do not apply stimulation when in bath or shower.
- 8) Do not apply stimulation while sleeping.
- 9) Do not apply stimulation while driving, operating machinery, or during any activity when electrical stimulation can put you at risk of injury.

- 10) Apply stimulation only to normal, intact, clean, healthy skin.
- 11) The long-term effects of electrical stimulation are unknown. Electrical stimulation device cannot replace drugs.
- 12) Stimulation should not take place while the user is connected to high-frequency surgical equipment, which may cause burn injuries on the skin under the electrodes, as well as problems with the stimulator.
- 13) Do not use the stimulator in the vicinity of shortwave or microwave therapy equipment, since this may affect the output power of the stimulator.
- 14) Never use it near the cardiac area. Stimulation electrodes should never be placed anywhere on the front of the thorax (marked by ribs and breastbone), but above all not on the two large pectoral muscles. There it can increase the risk of ventricular fibrillation and lead to cardiac arrest. 
- 15) Never use it on the eye, head and face area. 
- 16) Never use it near the genitals.
- 17) Never use it on the areas of the skin which lack normal sensation
- 18) Keep electrodes separate during treatment. It could result in improper stimulation or skin burns if electrodes are in contact with each other.
- 19) Keep the stimulator out of reach of children.
- 20) Consult your doctor if you are in any doubt whatsoever.
- 21) Discontinue it and do not increase the intensity level if you feel discomfort during use.

2.2.3 Precautions

- 1) TENS is not effective for pain of central origin including headache.
- 2) TENS is not a substitute for pain medications and other pain management therapies.
- 3) TENS is a symptomatic treatment and, as such, suppresses the sensation of pain that would otherwise serve as a protective mechanism.
- 4) Effectiveness is highly dependent upon patient selection by a practitioner qualified in the management of pain patients.
- 5) Since the effects of stimulation of the brain are unknown, stimulation should not be applied across your head, and electrodes should not be placed on opposite sides of your head.
- 6) The safety of electrical stimulation during pregnancy has not been established.
- 7) You may experience skin irritation or hypersensitivity due to the electrical stimulation or electrical conductive medium (silica gel).
- 8) If you have suspected or diagnosed heart disease or epilepsy, you should follow precautions recommended by your physician.
- 9) Caution if you have a tendency to bleed internally, e.g. following an injury of fracture.
- 10) Consult with your physician prior to using the device after a recent surgical procedure, because stimulation may disrupt the healing process.
- 11) Caution if stimulation is intended to be applied over the menstruation or pregnant uterus.
- 12) For single patient use only.

- 13) This stimulator should not be used by patients who is noncompliant and emotionally disturbed including whom with dementia or low IQ.
- 14) The instruction of use is listed and should be obeyed; any improper use may be dangerous.
- 15) Rare cases of skin irritation may occur at the site of the electrode placement following long-term application.
- 16) Do not use this device in the presence of other equipment which sends electrical pulses to your body.
- 17) Do not use sharp objects such as a pencil or ballpoint tip to operate the buttons on the control panel.
- 18) Check the electrode connections before each use.
- 19) Electrical stimulators should be used only with the electrodes recommended for use by the manufacturer.
- 20) When output of device more than 10mA or 10 V, the intensity of Channel will flicker.
- 21) Users should consult a healthcare professional before using the device.
- 22) The user shall report any serious incident related to the device to the manufacturer and the competent authorities of the Member States establishing the user and / or the patient.

2.2.4 Adverse Reactions

- 1) Possible skin irritation or electrode burn under the electrodes may occur.
- 2) Possible allergic skin reaction to tape or gel may occur.
- 3) On very rare occasions, first-time users of EMS report feeling light-headed or faint. We recommend that you use the product while seated until you become accustomed to the sensation.
- 4) If symptoms of tachycardia and extrasystolia (rapid heartbeat or extra stimulation) appear during treatment, stop the treatment and seek medical attention immediately.


- 5) If the stimulation makes you uncomfortable, reduce the stimulation Intensity to a comfortable level and contact your physician if problems continue.

3. GETTING TO KNOW YOUR DEVICE

3.1 Package includes

No.	Description	QTY
1	The Stimulator	1pc
2	Electrode pad (50mm×50mm)	4pcs
3	Electrode wires	2pcs
4	Ordinary batteries (1.5V, AAA)	4pcs
5	User manual	1pc


3.2 LCD display

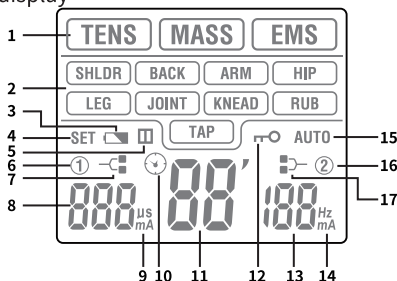

No.	Function description	No.	Function description
1	Treatment mode	10	Timer sign
2	Treatment body part	11	Standby mode: program number; Working mode: treatment time
3	Low battery indicator	12	Key locking symbol
4	SET Sign	13	intensity of Channel2
5	PAUSE Sign	14	Unit of treatment intensity for Channel 2

6	Symbol of Channel 1	15	AUTO Sign
7	Indicator of no load (Channel 1)	16	Symbol of Channel 2
8	intensity of Channel1.	17	Indicator of no load (Channel 2)
9	Unit of treatment intensity for Channel 1		

3.3 Device illustration

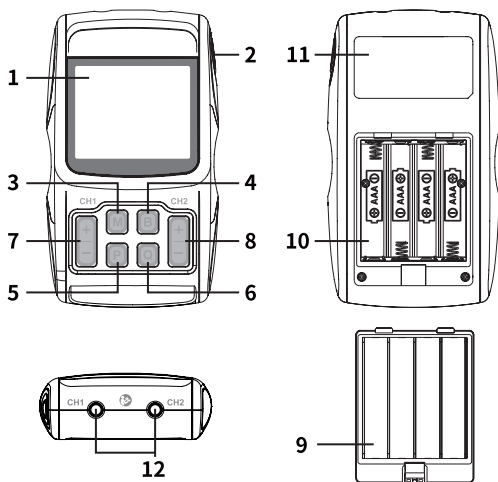

No.	Description
1	LCD display
2	[ON/OFF] button: At power saving mode, press the [ON/OFF] button to turn on the device; At standby mode, press the [ON/OFF] button to turn off the device; At treating mode, press the [ON/OFF] button to stop the treatment. At query mode, press the [ON/OFF] button to standby mode.
3	[M] button: At standby mode, press the [M] button to select the treatment mode.

4	[B] button: At standby mode, press the [B] button to select the treatment body part.
5	[P] button: At standby mode, press the [P] button to select the treatment program.
6	[Q] button: At standby mode, press the [Q] button to query the treatment records. In treatment mode, press [Q] to pause the treatment.
7	[+] button: At standby mode, press the [+] button to increase the CH1 and CH2 output intensity;
8	[-] button: At standby mode, press the [-] button to decrease the CH1 and CH2 output intensity; At the key locking mode, press the [-] button to unlock the keys.
9	Battery cover
10	Battery compartment
11	Rating label
12	Output socket

4. SPECIFICATION

4.1 Technical information

Device name	Electrotherapy unit
Model/type	R-C1
Power supply	6.0 V D.C., 4x AAA batteries
Output Channel	Dual channel
Waveform	Bi-phase square-wave pulse
Output voltage	Max. 120V _{pp} (at 1000ohm load)
Output current	Max. 60mA (at 1000ohm load)
Output intensity	0 to 60 levels, adjustable
Treatment mode:	TENS , EMS and MASSAGE mode
Output characteristics	Constant Current (CC)
Operating condition	5 ° C to 40 ° C with a relative humidity of 15%-93%, atmospheric pressure from 700 hPa to 1060 hPa
Storage condition	-10 ° C to 55 ° C with a relative humidity of 10%-95%, atmospheric pressure from 700 hPa to 1060 hPa
Dimension	120.5x69.5x27 mm (L x W x T)
Weight	104g(without battery)

Automatic shutoff	3 minutes
Classification	BF type applied part, internal power equipment, IP22
Electrode detection function	The electric current level will be reset to 0 mA, when the amplitude level is 9 or greater and an open circuit at either channel is detected.
Size of electrodes pad	50x50mm, square
Output precision	$\pm 20\%$ error is allowed for all the output parameters
Device service life	5 years
Electrode pads shelf life	3 years

TENS mode

Number of program	18 programs
P.W. (pulse width)	100-330 μ s
P.R. (Frequency)	2-125Hz (Hz=vibration per second)
Burst frequency	2Hz
Treatment time	30 minutes

EMS mode

Number of program	15 programs
P.W. (pulse width)	200-280 μ s
P.R. (Frequency)	1-70 Hz (Hz=vibration per second)
Treatment time	28 and 32 minutes

MASSAGE mode


Number of program	3 programs
P.W. (pulse width)	30-220 μ s
P.R. (Frequency)	25-100Hz (Hz=vibration per second)
Treatment time	30 minutes

5. OPERATING INSTRUCTION

5.1 Battery

5.1.1 Check/ replace batteries

Open the battery cover, insert four batteries (type AAA) into the battery compartment. Make sure you are installing the batteries properly. Be sure to place the batteries according to the markings of positive end(+) and negative end (-) in the battery compartment of device.



Open the battery cover, insert four batteries (type AAA) into the battery compartment. Make sure you are installing the batteries properly. Be sure to place the batteries according to the markings of positive end(+) and negative end (-) in the battery compartment of device.

5.1.2 Disposal of battery

Spent batteries do not belong to the household waste. Dispose of the battery following the current regulations. As a consumer, you have legal obligation to return spent battery to the Recycle Bin.



Caution

1. If a battery was swallowed accidentally, please seek medical assistance immediately !
2. In case of battery leakage, please avoid contact with the battery through skin, eyes and mucus membranes. Once it occurs , please wash the contacted part with plenty of clean water and contact your doctor immediately.
3. Battery cannot be dismantled, thrown into fire or short-circuited.
4. Protect battery from excess heat; Take the battery out of the product if they are spent or you don' t use it for a long time. This can prevent device damage due to the battery leakage.
5. Replace all of the batteries simultaneously!
6. Always replace the device with the same type battery.

5.2 Connect electrode pads to electrode wires

Insert the electrode wires connector into electrode connector. Make sure they are properly connected to ensure the good performance. Please refer to the picture.



Caution

Always use the electrode pads which comply with the requirements of the IEC/EN60601-1, ISO10993-1/-5/-10 and IEC/ EN60601-1-2, as well as CE and FDA 510(K) regulation.

5.3 Connect electrodes wires to device

Before proceeding to this step, be sure the device is completely switched OFF.

Hold the insulated portion of the electrode wire connector, and insert the plug into the receptacle on the top of the main device.



Ensure the electrode wires are inserted correctly. The device has two output receptacles controlled by Channel A and Channel B at the top of the unit. You may choose to use one channel with one pair of electrode wires or both channels with two pairs of electrode wires. Using both channels gives the user the advantage of stimulating two different areas at the same time.

Caution

Do not insert the plug of the electrode wires into any AC power supply socket.

5.4 Electrode

5.4.1 Electrode options

The electrodes are disposable and should be routinely re-

placed when they start to lose their adhesiveness. If you are unsure of your electrode adhesive properties, please order new replacement electrodes. Replacement electrodes should be re-ordered under the advice of your physician or the device manufacturer to ensure proper quality. Follow application procedures outlined on electrode packings when using the new replacement electrodes to maintain optimal stimulation and to prevent skin irritation.

5.4.2 Place electrodes on skin

Place the electrode on the body part in need of treatment, according to the instruction of this user manual. Please make the skin clean before use and ensure the skin and electrode connect well.



Caution




1. Always remove the electrodes from the skin with a moderate pull in order to avoid injury in the event of highly sensitive skin.
2. Before applying the self-adhesive electrodes, it is recommended to wash and degrease the skin, and then dry it.
3. Do not turn on the device when the self-adhesive electrodes are not positioned on the body.
4. To remove or move the electrodes, switch off the device or the appropriate channel first in order to avoid unwanted irritation.
5. It is recommended that, at minimum, 1.97" x 1.97" self-adhesive square electrodes are used at the treatment area.
6. Never remove the self-adhesive electrodes from the skin while the device is still on.





5.4.3 Electrode placement

The R-C1 is a kind of OTC stimulator, suitable for home use. You only have to use according to the user manual, place the electrode on the position where you feel pain. Conducting exercise, treatment and adjustment based on your own feeling.

Different programs with corresponding applicable symptoms as below:





Position of electrode placement under TENS programs

Shoulder	
Back	
Arm	
	

Leg	       
Joint	  
Joint	 
Hip	   

Position of electrode placement under EMS programs

Arm	 
-----	---


Back	
Leg	
Shoulder	
Hip	

6. INSTRUCTIONS FOR USE

6.1 Turn on


When use it for the first time, open the battery cover and load four new batteries (Please kindly review Section 5.1.1 for the operating steps and schematic diagram)

Press the [ON/OFF] button to turn the device on, the LCD will be lit. And then it goes into the standby mode as below picture shows.

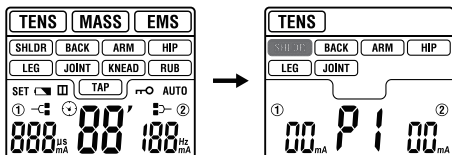


6.2 Select treatment mode

Press the [M] button to select which treatment mode (TENS --MASS- EMS) you will use. The LCD displays as follows:

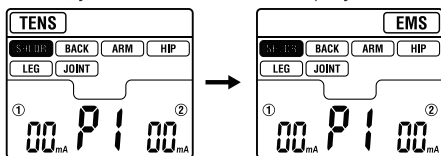


6.3 Select treatment body part

Based on your needs, press [B] button to select the current treatment body part. Press each [B] button to switch body part. The LCD displays as follows:

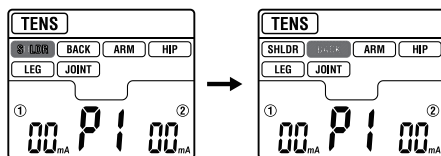


6.4 Select treatment program

Based on your needs, press [P] button to select the treatment program. For each body part, it has 3 treatment programs. The LCD displays as follows:

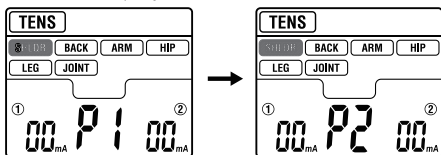


6.5 Start treatment

Press the [+] button of CH1 to increase the channel 1 intensity, press the [+] button of CH2 to increase the channel 2 intensity. The LCD displays as follows:

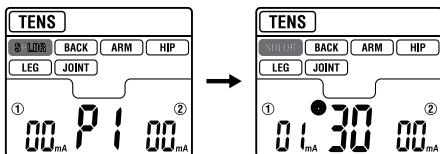


6.6 Adjust the output intensity

Place the electrodes on the body parts, press the [+] button to increase output intensity. It will be increased to a higher level after each press. The device has totally 60 levels of output intensity. Please adjust the intensity to the condition that you feel comfortable. The level of output intensity will be shown on the LCD:

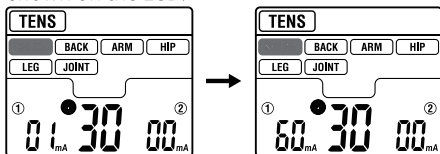

If you feel it too strong, you can press [-] button to decrease the intensity to a lower level each time. When the output intensity of both channels decrease to zero, the stimulator will return to the standby mode. The LCD displays as follows:

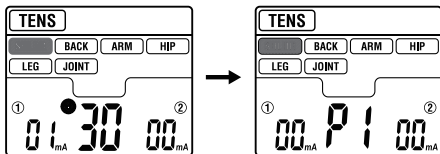


Caution:

If you feel or become uncomfortable, reduce the stimulation intensity to a more comfortable level and consult with your medical practitioner if problems insist.


6.7 Pause the treatment

On the treating mode, press the [Q] button to pause the treatment, and the LCD will display the icon **⏸**. Press the [Q] button again to regain the treatment.



6.8 Stop the treatment and turn off the device

Press the [ON/OFF] button to stop treatment during the treating mode. Press the [ON/OFF] button again to turn off the stimulator, and the LCD will be blank.

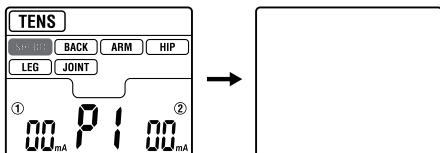

6.9 Key Lock Function

After adjustment is complete, if no key is pressed within 20 seconds, the device will automatically lock the keys **⏹** to prevent accidental touches.


The [ON/OFF] key does not lock, making it convenient to stop the output intensity in an emergency.

There are two ways to unlock: short press the [-] (CH1/CH2) key, or wait for the device to automatically unlock after the treatment ends.




6.10 Load detection

It will automatically detect the load if the intensity is above Level 9.If it haven't detected the load or the electrode contacts the skin not well enough ,the intensity will automatically return to Level 0 and the symbol  twinkles. And the stimulator returns to the standby mode.



6.11 Query the treatment records

If you want to query the treatment records, press the [Q] button to check the details. The LCD will show as follows:

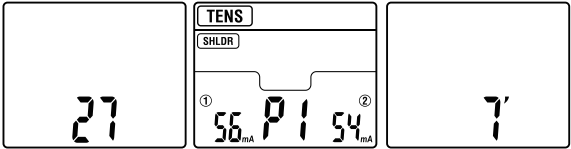


Press the [+] button or [-] button to view the treatment history.

Press the [ON/OFF] button to return to the standby mode.

6.12 Low battery detection

When the battery is low, the icon  will twinkle to indicate it. You should follow the Section 5.1.1 to replace batteries.



Notice of batteries:

- Batteries may be fatal if swallowed. Therefore, keep the batteries and the product out of the reach of children. If a battery is swallowed, go to a hospital immediately.
- If there's battery leakage, avoid contact with skin, eyes and mucus membranes. Rinse the affected spots with plenty of clear water immediately and contact a physician right away.
- Batteries must not be charged, dismantled, thrown into fire or short-circuited.
- Protect batteries from excess heat. Take the batteries out of the device if they are spent or in case that you will no longer use the them. This prevents damage caused by leaking batteries.

6.13 Usage of electrode pads

- The electrode may only be connected with **this** stimulator. Make sure that the device is turned off when attaching or removing the electrode pads.
- If you want to reposition the electrode during the application, turn the device off first.
- The use of electrode may lead to skin irritations. If you experience such skin irritations, e.g. redness, blistering or itching, discontinue using them. Do not use permanently on the same body part, as this may also lead to skin irritations.
- Electrode pads are private and intended for single person use. Please avoid use them by different persons.

- e. The electrode must connect entirely to the skin surface to prevent hot spots, which may lead to skin burns.
- f. Do not use the electrode pads for more than approx. 15 times, as connection between the electrodes and the skin deteriorates over time.
- g. The adhesive force of the electrodes depends on the skin properties, storage condition, and the number of applications. If your electrode pads no longer fully stick to the skin's surface, replace them with new ones. Stick the electrode pads back onto the protective foil after use and store them in the storage bag to prevent them from drying out. This retains the adhesive force for a longer period.
- h. Do not use detergent to clean the electrode pads before and after use to avoid damaging the adhesion of the electrode pads.
- i. The electrode pads must always be touched with clean hands, it is recommended to replace the electrode pads if they become dirty.

Caution:

- 1) Before applying the electrode, it is recommended for users to wash and degrease the skin, and then dry it.
- 2) Never remove the electrode from the skin while the device is still on.
- 3) Only use the electrode pads provided by the manufacturer. Use of other companies' products could result in injuries to the user.

6.14 Where do I attach electrode pads?

- a. Each person reacts differently to electric nerve stimulation. Therefore, the placement of the electrodes may deviate from the standard. If application is not successful, contact your physician to find out which placement techniques are best for you.
- b. Do not use any adhesive electrodes with a size smaller than those the original manufacturer attached. Otherwise the current density may be too high and cause injuries.
- c. The size of the adhesive pads may not be changed, e.g. by clipping off parts of them.
- d. Make sure that the region radiating the pain is enclosed by the electrodes. In case of painful muscle groups, attach the electrodes in such a way that the affected muscles are also enclosed by the electrodes.

Usage advice for TENS:

- a) If you feel the output intensity too strong, you can press [-] button to decrease it;
- b) During the treatment if you don't feel any discomfort, we advise you use the device until the session ends. Normally, the pain relief occurs after 5~10 mins treatment;
- c) Normally, we advise 1~2 treatments per day and one week as a period of treatment;
- d) After a period of treatment, if the pain relief is not achieved or the pain gets even worse, please consult your doctor.

7. Program

7.1 Treatment program

In TENS mode

Appli- cable parts	Pro- gram	Wave- form	Frequency(Hz)	Pulse Width (uS)	Treat time (Min.)
Shoul- der	P1	FM	2/4/6	250	30
	P2	FM	4/5/6/8	250	30
	P3	FM&PM	2-125	100-200	30
Back	P1	FM	60/55/10/50/45	200	30
	P2	FM	6/8/10	250	30
	P3	PM	55	330/ 150	30
Arm	P1	Continuous	2	250	30
	P2	Han	2/100	200/150	30
	P3	IM	100	200	30
Hip	P1	Burst	100	150	30
	P2	FM	4/6/50	250	30
	P3	IM	100	200	30
Leg	P1	FM	4/6/50	250	30
	P2	Burst	100	150	30
	P3	FM	6/8/10	250	30
Joint	P1	Han	2/100	200/150	30
	P2	Burst	100	150	30
	U1	Continuous	80	150	30

In EMS mode

Appli- cable parts	Pro- gram	Wave- form	Frequency(Hz)	Pulse Width (uS)	Treat time (Min.)
Shoulder	P1	Synchronous	5/50/6/3	280	28
	P2	Synchronous	5/60/4/3	280	32
	P3	Synchronous	5/70/1/3	280	32
Back	P1	Synchronous	5/50/6/3	250	28
	P2	Synchronous	5/60/4/3	250	32
	P3	Synchronous	5/70/1/3	250	32
Arm	P1	Synchronous	5/50/6/3	200	28
	P2	Synchronous	5/60/4/3	200	32
	P3	Synchronous	5/70/1/3	200	32
Hip	P1	Synchronous	5/50/6/3	250	28
	P2	Synchronous	5/60/4/3	250	32
	P3	Synchronous	5/70/1/3	250	32
Leg	P1	Synchronous	5/50/6/3	200	28
	P2	Synchronous	5/60/4/3	200	32
	P3	Synchronous	5/70/1/3	200	32

In massage mode

Appli- cable parts	Pro- gram	Wave- form	Frequency(Hz)	Pulse Width (uS)	Treat time (Min.)
Knead	P1	FM&PM	28~45	50~220	30
Rup	P1	FM&PM	25~80	30~220	30
Tap	P1	FM&PM	49~100	30~220	30

8. Cleaning and maintenance

Fully comply with the following necessary daily maintenance requirements to make sure the device is intact and guarantee its long term performance and safety.

8.1 Cleaning and care for the device

8.1.1 Pull the electrodes out of the stimulator, remove the batteries and clean the device with a soft, slightly damp cloth. In case of heavier dirt build-up, you may also apply a mild detergent.

8.1.2 Do not expose the stimulator to moisture or dampness. Do not hold the stimulator under running water, nor submerge it in water or other liquids.

8.1.3 The stimulator is sensitive to heat and may not be exposed to direct sunlight. And do not place it on hot surfaces.

8.1.4 Clean the surface of the electrode pads carefully with a damp cloth. Make sure the device is turn off!

8.1.5 For reasons of hygiene, each user should use his/her own set of electrodes.

8.1.6 Do not use any chemical cleaners or abrasive agents for cleaning.

8.1.7 Ensure that no water penetrates into the machine. Should this happen, use the device again only when it is completely dry.

8.1.8 Do not clean the device during treatment. Be sure that the device is turned off and the battery is unloaded before cleaning.

8.2 Maintenance

- 8.2.1 The manufacturer didn't authorize any maintenance agencies abroad. If your device has any problem, please contact the distributor. The manufacturer will not be responsible for the results of maintenance or repairs by unauthorized persons.
- 8.3.2 The user must not attempt any repairs to the device or any of its accessories. Please contact the retailer for repair.
- 8.3.3 Opening of the equipment by unauthorized agencies is not allowed and will terminate any claim to warranty.

Each product in manufacturing has been through the systematic validation. The performance is stable and does not need to undertake calibration and validation.

If your product can't reach the expected performance and the basic function has changes in normal use, please contact the retailer.

9. Troubleshooting

Should any malfunction occur while using the device, check whether the parameters are set appropriately for therapy, and adjust the control correctly. Please see the following table:

Malfunction	Common reasons	Countermeasure
No display after replacing the battery.	1. There's foreign body in the battery compartment. 2. The battery has been used up or installed oppositely. 3. There is foreign body in the battery interface. 4. The battery is not the right model or something goes wrong with the battery interface 5. Exception reset	1. Check and clean the compartment. 2. Replace the new battery or install the battery correctly. 3. Check and clean the interface. 4. Replace the battery with the right model.
No sensation of stimulation or weak stimulation	1. The electrode does not connect well to the skin. 2. If the connect between electrode connect well to the stimulator. 3. The battery is used up. 4. The skin is too dry.	1. Check and re-paste it on skin. 2. Check the connection.. 3. Replace the battery. 4. Wipe the electrode and the skin with a wet cotton cloth.

Automatic halt in the treatment	1. The electrode loses connection with the skin. 2. If the battery is used up.	1. Check and place the electrode properly on the skin. 2. Replace the battery.
Rash or tickle on the skin occurs in treatment	1. The treatment time lasts too long. 2. The electrode does not stick well to the skin. 3. The interface of the electrodes is dirty or dry. 4. The skin is sensitive to the electrode.	1. Do the treatment once a day and shorten the treatment time. 2. Check and stick the electrode well. 3. Wipe the electrode with a wet cotton cloth before use. 4. Check your allergic history. Please change the sticking place or shorten the treatment time .If your skin is over-sensitive, you should stop the treatment or go to see a doctor.

10. Storage

Remove the batteries from the device if you are not going to use it for a long period. Battery leakage can damage the unit. Do not make any sharp pull-out between the connection of the leadwires and the electrodes. After use, put the electrode away in the original package. Do not expose the device to direct sunlight and protect it against dirt and moisture. Store the machine in a cool, well-ventilated place. Never place any heavy objects over the machine.

11. Disposal

Spent batteries do not belong to the household wastes. Dispose of the battery according to the current regulations. As a consumer, you have the obligation to dispose of batteries correctly. Consult your municipal authority or your dealer for information about disposal.

At the end of the product lifecycle, do not throw this product into the normal household garbage, but bring it to a collection point for the recycling of electronic equipment. Obsolete electrical and electronic equipment may have potentially harmful effects on the environment. Incorrect disposal can cause toxins to build up in the air, water and soil and jeopardize human health.

12. Electromagnetic compatibility (EMC) tables

Guidance and manufacture's declaration - electromagnetic emissions		
The device is intended for use in the electromagnetic environment specified below. The customer or the user has to assure that it is used in such environment.		
Emissions test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR11	Group 1	The device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.

RF emissions CISPR11	Class B	The device is suitable for use in all establishments including those directly connected to the public low-voltage power supply network that supplies to buildings power used for domestic purposes
Harmonic emissions IEC61000-3-2	Not applicable	
Voltage fluctuations/ Flicker emissions IEC61000-3-3	Not applicable	

Guidance and manufacture's declaration — electromagnetic immunity

The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such environment.

Immunity test	IEC 60601 Test level	Compliance level	Electromagnetic environment-guidance
Electrostatic discharge (ESD) IEC61000-4-2	$\pm 8\text{kV}$ direct & indirect contact; $\pm 15\text{kV}$ air discharge	$\pm 8\text{kV}$ direct & indirect contact; $\pm 15\text{kV}$ air discharge	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%
Electrical fast transient/burst IEC 61000-4-4	$\pm 2\text{ kV}$ for power supply lines	not applicable	not applicable (for INTERNALLY POWERED ME EQUIPMENT)
Surge IEC 61000-4-5	$\pm 1\text{ kV}$ line(s) to line(s)	not applicable	not applicable (for INTERNALLY POWERED ME EQUIPMENT)

Voltage dips, short interrup- tions and volt- age variations on power supply input lines IEC 61000-4-11	$<5\% U_T$ ($>95\%$ dip in U_T) for 0.5 cycle $40\% U_T$ (60% dip in U_T) for 5 cycles $70\% U_T$ (30% dip in U_T) for 25 cycles $<5\% U_T$ ($>95\%$ dip in U_T) for 5 sec	not applica- ble	not applicable (For INTERNAL- LY POWERED ME EQUIPMENT
---	---	---------------------	--

Power frequency (50Hz/60Hz) magnetic field IEC 61000-4-8	10V/m	10V/m	Power frequency mag- netic fields should be at levels characteristic of a typical location in a typical commercial or hospital environ- ment.
---	-------	-------	---

NOTE U_T is the a.c. mains voltage prior to application of the test level.

Guidance and manufacture' s declaration – electromagnetic im-
munity

The device is intended for use in the electromagnetic environment
specified below. The customer or the user of device should assure
that it is used in such an environment.

Immunity test	IEC 60601 test level	Compli- ance level	Electromagnetic environment - guidance
------------------	-------------------------------	-----------------------	---

Radiated RF IEC 61000-4-3	10V/m & table 9	10V/m & table 9	Portable and mobile RF communications equipment should be used not closer to any part of the Blood Pressure Monitor, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d = 1.167\sqrt{P}$ 80 MHz to 800 MHz $d = 2.333\sqrt{P}$ 800 MHz to 2.5 GHz Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,^a should be less than the compliance level in each frequency range.^b Interference may occur in the vicinity of equipment marked with the following symbol: 
NOTE 1	At 80 MHz and 800 MHz, the higher frequency range applies.		
NOTE 2	These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.		

- a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Blood Pressure Monitor is used exceeds the applicable RF compliance level above, the Blood Pressure Monitor should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the Blood Pressure Monitor.
- b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than [Vi] V/m.

Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment (Table 9)

Test frequency (MHz)	Band ^{a)} (MHz)	Service ^{a)}	Modulation ^{b)}	Maximum power (W)	Distance (m)	Immunity Test Level (V/m)
385	380-390	TETRA 400	Pulse modulation ^{b)} 18Hz	1.8	0.3	27
450	430-470	GMRS 460, FRS 460	FM ^{c)} ± 5 kHz deviation 1kHz sine	2	0.3	28
710	704-787	LTE Band 13, 17	Pulse modulation ^{b)} 217Hz	0.2	0.3	9
745						
780						
810	800-960	GSM800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation ^{b)} 18Hz	2	0.3	28
870						
930						

1720	1700-1990	GSM1800; CDMA 1900; GSM 1900; DECT; LTE Band 1,3, 4,25; UMTS	Pulse modu- lation ^{b)} 217Hz	2	0.3	28
1845						
1970						
2450	2400-2570	Bluetooth, WLAN, 802.11 b/g/ n, RFID 2450, LTE Band 7	Pulse modu- lation ^{b)} 217Hz	2	0.3	28
5240	5100-5800	WLAN 802.11 a/n	Pulse modu- lation ^{b)} 217Hz	0.2	0.3	9
5500						
5785						

NOTE If it is necessary to achieve the IMMUNITY TEST LEVEL, the distance between the transmitting antenna and the ME EQUIPMENT or ME SYSTEM may be reduced to 1 m. The 1 m test distance is permitted by IEC 61000-4-3.

- a) For some services, only the uplink frequencies are included.
- b) The carrier shall be modulated using a 50 % duty cycle square wave signal.
- c) As an alternative to FM modulation, 50 % pulse modulation at 18 Hz may be used because it does not represent actual modulation. It would be worst case.

13. Normalized symbols

	WEEE Symbol		Applied part of type BF
	Refer to instruction manual	IP22	IP classification
LOT	Batch code	EU REP	Authorized representative in the European Community
	Manufacturer		Date of manufacture
	Fragile, handle with care		Keep away from sunlight
	Keep dry		Temperature limit
	Use-by date	SN	Serial number
	Humidity limitation		Atmospheric pressure limitation
	Caution		Recycling symbol
	Users of the artificial pacemaker are prohibited from using the device	CE 2460	CE mark
	Packaging material cycle mark	MD	Medical device
UDI	Unique device identifier		Importer

14. WARRANTY

Please contact your dealer or the device centre in case of a claim under the warranty. If you have to return the unit, enclose a copy of your receipt with clear statement of defect description.

The warranty terms is below:

1. The warranty period for this device is 1 year from date of purchase. In case of a warranty claim, the date of purchase has to be proven by means of the sales receipt or invoice.
2. Repairs under warranty should be in the warranty period either for the device or for the replacement parts.
3. The following cases are excluded under the warranty
 - All damages that arise due to improper operation, e.g. nonobservance of the user instruction.
 - All damages due to repairs or tampering by the customer or unauthorized third parties.
 - Damage which has arisen during transport from the manufacturer to the consumer or the service centre.
 - Accessories which are subject to normal wear and tear.
 - Device damage due to privately disassembling devices.
4. Liability for direct or indirect consequential losses caused by the unit is excluded even if the damage to the unit is accepted as a warranty claim



