



GIMA
PROFESSIONAL MEDICAL PRODUCTS

OXY-2 FINGER OXIMETER

Use and maintenance book

ATTENTION: Operators must read and understand this manual completely before using the product.

GIMA 35072

CONTEC MEDICAL SYSTEMS CO., LTD No.112
Chunzhang West Street, Economic & Technical
Development Zone, Chihuahua, Hebei Province,
PEOPLE'S REPUBLIC OF CHINA
Made in China

REF CMS500L

Proline GmbH, Brehmstr. 56, 40239
Duesseldorf Germany

Gima S.p.A.
Via Marconi, 1 - 20060 Gessate (MI) Italy
gima@gmail.com - export@gimaitaly.com
www.gimaitaly.com

CMS2.782.446(CE)SS/1.3 1.4.01.51.316 2025.05



User Notice

Dear users, thank you very much for purchasing the Pulse Oximeter (hereinafter referred to as device).

This Manual is written and compiled in accordance with the council directive MDD93/42/EEC for medical devices and harmonized standards. In case of modifications and software upgrades, the information contained in this document is subject to change without notice.

It is a medical device, which can be used repeatedly.

The Manual describes, in accordance with the device's features and requirements, main structure, functions, specifications, correct methods for transportation, assembly, usage, operation, repair, maintenance and storage, etc. as well as the safety procedures to protect both the user and device. Refer to the respective chapters for details.

Please read the User Manual carefully before using this device. The User Manual which describes the operating procedures should be followed strictly. Failure to follow the User Manual may cause measuring abnormality, device damage and human injury. The manufacturer is NOT responsible for the safety, reliability and performance issues and any monitoring abnormality, human injury and device damage due to users' negligence of the operation instructions. The manufacturer's warranty service does not cover such faults.

Owing to the forthcoming renovation, the specific products you received may not be totally in accordance with the description of this User Manual. We would sincerely regret for that.

Our company has the final interpretation to this manual. The content of this manual is subject to change without prior notice.

Warnings

Remind that it may cause serious consequences to tester, user or environment.

- Explosive hazard—DO NOT use the device in environment with inflammable gas such as anesthetic.
- DO NOT use the device while examining by MRI or CT, as the induced current may cause burn.
- Do not take the information displayed on the device as the sole basis for clinical diagnosis. The device is only used as an auxiliary means in diagnosis. And it must be used in conjunction with doctor's advice, clinical manifestations and symptoms.
- The maintenance to the device. Users are not permitted to maintain or refit the device by themselves.
- Uncomfortable or painful feeling may appear if using the device ceaselessly, especially for the microcirculation disturbance users. It is not recommended that the sensor is used on the same finger for more than 2 hours.
- For some special users who need a more careful inspection on the test site, please don't place the device on the edema or tender tissue.
- Please do not stare at the red and infrared light emitter (the infrared light is invisible) after turning on the device, including the maintenance staff, as it may be harmful to the eyes.
- Each part of the device is firmly fixed, if accidental falling leads to the small parts such as a button to fall off, avoid swallowing of these parts, it may cause suffocation.
- The device contains silicone, PVC, TPU, TPE and ABS materials, whose biocompatibility has been tested in accordance with the requirements in ISO 10993-1, and it has passed the recommended biocompatibility test. The person who is allergic to silicone, PVC, TPU, TPE or ABS can not use this device.
- Do NOT strand the lanyard to avoid device drop and damage. The lanyard is made of insensitive material. Please do not use it if any person is allergic to lanyard. Do

- not wrap the lanyard around neck to avoid an accident.
- The disposal of scrap device, its accessories and packaging should follow the local laws and regulations, to avoid polluting to the local environment. And the packaging materials must be placed in the region where the children are out of reaching.
- The device can not be used with the equipment not specified in the Manual. Only the accessories appointed or recommended by the manufacturer can be used, otherwise it may cause injury to the tester and operator or damage to the device.
- Check the device before use to make sure that there is no visible damage that may affect user's safety and device performance. When there is obvious damage, please replace the damaged parts before use.
- Functional testers can not be used to assess the accuracy of the Pulse Oximeter.
- Some functional testers or patient simulators can be used to verify whether the device works normally, for example, INDEX-2LFE Simulator (software version: 3.00), please refer to the Manual for the detailed operation steps.
- Some functional testers or patient simulators can measure the accuracy of the device copied calibration curve, but they can not be used to evaluate the device accuracy.
- When using the device, please keep it away from the equipment which can generate strong electric field or strong magnetic field. Using the device in an inappropriate environment may cause interference to the surrounding radio equipment or affect its working.
- When storing the device, keep it away from children, pets and insects to avoid affecting its performance.
- Do not place the device in places exposed to direct sunlight, high temperature, humidity, dust, cotton wool or easy to splash water, to avoid affecting its performance
- The measured accuracy will be affected by the interference of electrosurgical equipment.
- When several products are used on the same patient simultaneously, danger may occur which is arisen from the overlap of leakage current.
- CO poisoning will appear excessive estimation, so it is not recommended to use the device.
- This device is not intended for treatment.
- The intended operator of the device may be a patient.
- Avoid maintaining the device during using.
- Users should read the product manual carefully before use and operate according to the requirements.

1 Overview

The oxygen saturation is the percentage of HbO₂ in the total Hb in the blood, so-called the O₂ concentration in the blood, it is an important physiological parameter for the respiratory and circulatory system. A number of diseases related to respiratory system may cause the decrease of SpO₂ in the blood, furthermore, some other causes such as the malfunction of human body's self-adjustment, damages during surgery, and the injuries caused by some medical checkup would also lead to the difficulty of oxygen supply in human body, and the corresponding symptoms would appear as a consequence, such as vertigo, impotence, vomit etc. Serious symptoms might bring danger to human's life. Therefore, prompt information of patients' SpO₂ is of great help for the doctor to discover the potential danger, and is of great importance in the clinical medical field.

Insert the finger when measuring, the device will directly display the SpO₂ value measured, it has a higher accuracy and repeatability.

1.1 Features

- Easy to use.
- Small in volume, light in weight, convenient to carry.
- Low power consumption.

1.2 Applied range

The Pulse Oximeter can be used in measuring the pulse oxygen saturation and pulse rate through finger. The product is suitable for being used in family, hospital, oxygen bar, community healthcare, physical care in sports (It can be used before or after doing sports, and it is not recommended to use the device during the process of having sport) and etc.

1.3 Environment requirements

Storage Environment

- Temperature: -40 °C ~ + 60 °C
- Relative humidity: ≤ 95%
- Atmospheric pressure: 500 hPa ~ 1060 hPa

Operating Environment

- Temperature: +10 °C ~ + 40 °C
- Relative Humidity: ≤ 75%
- Atmospheric pressure: 700 hPa ~ 1060 hPa

1.4 Precautions

1.4.1 Attention

Point out conditions or practices that may cause damage to the device or other properties.

- Before using the device, make sure that it locates in normal working state and

- operating environment.
 - In order to get a more accurate measurement, it should be used in a quiet and comfortable environment.
 - When it is carried from cold environment to warm or humid environment, please do not use it immediately.
 - If the device is splashed or coagulated by water, please stop operating.
 - DO NOT operate the device with sharp things.
 - High temperature, high pressure, gas sterilizing or immersion disinfection for the device is not permitted. Refer to User Manual in the relative chapter (6.1) for cleaning and disinfection..Please take out the internal battery before cleaning and disinfection.
 - The device is suitable for adult.
 - The device may not be suitable for all users, if you can't get a satisfactory result, please stop using it.
 - Data averaging and signal processing have a delay in the upgrade of SpO₂ data values. When the data update period is less than 30 seconds, the time for obtaining dynamic average values will increase, which is arisen from signal degradation, low perfusion or other interference, it depends on the PR value.
 - The device has 3-year service life, date of manufacture: see the label.
 - The device does not provide over-limit alarm function for SpO₂ and PR, so it is inapplicable for using in the place where need such function.
 - The device hasn't low-voltage prompt function, it only shows the low-voltage, please change the battery when the battery voltage is used up.
 - The maximum temperature at the SpO₂ probe -tissue interface should be less than 41°C which is measured by the temperature tester.
 - During measuring, when abnormal conditions appear on the screen, please pull out your finger and reinsert it to measure again.
 - If some unknown error appears during measuring, remove the battery to terminate operating.
 - Do not contort or drag the wire of the device.
 - The bar graph, as a signal inadequacy indicator, when it moves unsteadily, the accuracy of the measured value may degrade. When it tends to be steady, the measured value read is the optimal.
 - If the device or component is intended for single-use, then the repeated use of these parts will pose risks on the parameters and technical parameters of the equipment known to the manufacturer.
 - If necessary, our company can provide some information (such as circuit diagrams, component lists, illustrations, etc.), so that the qualified technical personnel of the user can repair the device components designated by our company.
 - Operators can contact our company to obtain the modified Bland and Altman plot.
 - The measured results will be influenced by the external colouring agent (such as nail polish, colouring agent or color skin care products, etc.), so don't use them on the test site.
 - Do not fix the SpO₂ sensor with adhesive or else it may result in venous pulsation and inaccurate measure of SpO₂ and pulse rate.
 - As to the fingers which are too cold or too thin or whose fingernail is too long, it may affect the measured results, so please insert the thicker finger such as thumb or middle finger deeply enough into the probe when measuring.
 - The finger should be placed correctly (see Attached figure 5), as improper assembly or improper contact position for sensor will influence the measurement.
 - The light between the photoelectric receiving tube and the light-emitting tube of the device must pass through the subject's arteriole. Make sure the optical path is free from any optical obstacles like rubberized fabric, to avoid inaccurate results.
 - Excessive ambient light may affect the measured results, such as surgical light (especially xenon light sources), bilirubin lamp, fluorescent lamp, infrared heater and direct sunlight, etc. In order to prevent interference from ambient light, make sure to place the sensor properly and cover the sensor with opaque material.
 - Frequent movement (active or passive) of the subject or severe activity can affect the measured accuracy.
 - The SpO₂ probe should not be placed on a limb with the blood pressure cuff, arterial ductus or intraluminal tube.
 - The measured value may be inaccurate during defibrillation and in a short period after defibrillation, as it has not defibrillation function.
 - The device has been calibrated before leaving factory.
 - The device is calibrated to display functional oxygen saturation.
 - The equipment connected with the Oximeter interface should comply with the requirements of IEC 60601-1.
- 1.4.2 Clinical restriction**
- A. As the measure is taken on the basis of arteriole pulse, substantial pulsating blood flow of subject is required. For a subject with weak pulse due to shock, raynaud's syndrome, low ambient/body temperature, major bleeding, or use of vascular contracting drug, the SpO₂

- waveform (PLETH) will decrease. In this case, the measurement will be more sensitive to interference.
- B. The measurement will be influenced by intravascular staining agents (such as indocyanine green or methylene blue), skin pigmentation.
- C. The measured value may be normal seemingly for the tester who has anemia or dysfunctional hemoglobin(such as carboxhaemoglobin (COHb), methaemoglobin (MetHb) and sulphaemoglobin (SuHb), but the tester may appear hypoxia, it is recommended to perform further assessment according the clinical situations and symptoms.
- D. Pulse oxygen only has a reference meaning for anemia and toxic hypoxia, as some severe anemia patients still show better pulse oxygen measured valued.
- E. Contraindication:
 - The person who is allergic to silicone, PVC, TPU TPE or ABS.
 - The damaged skin tissue.
 - During cardiopulmonary resuscitation.
 - When the patient is hypovolemic.
 - For assessing the adequacy of ventilatory support.
 - For detecting worsening lung function in patients on a high concentration of oxygen.

2 Principle

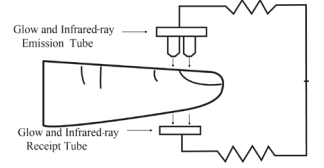


Figure 1 Operating principle

An experience formula of data processing is established taking use of Lambert Beer Law according to Spectrum Absorption Characteristics of Reductive Hemoglobin (Hb) and Oxhemoglobin (HbO₂) in red light & near-infrared light zones. On the basis of the principle of Photoelectric Oxyhemoglobin Inspection Technology and Photoplethysmography technology, it uses two light beams of different wavelengths to irradiate the human fingertip to obtain the measurement information from the photosensitive element, after processed by the electronic circuits and microprocessor, displays the measured results on the screen.

3 Functions

- SpO₂ value display
- PR value and bar graph display
- Low-battery indication: low-battery indication appears when the battery voltage is too low to work
- Automatic standby function

4 Product Introduction

4.1 View of the front panel

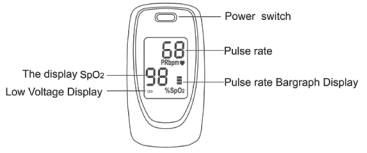


Figure 2. Front view

4.2 Battery

Step 1. Refer to Figure 3. and insert the two AAA size batteries properly in the right direction.

Step 2. Replace the cover.

Please take care when you insert the batteries for the improper insertion may damage the device.

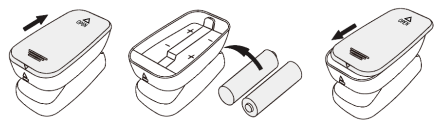


Figure 3. Batteries assembly

4.3 Mounting the hanging rope

- Step 1. Put the end of the rope through the hole.
- Step 2. Put another end of the rope through the first one and then tighten it.



Figure 4. Mounting the hanging rope.

4.4 Structure, accessories and software description

- A. Structure: main unit.
- B. Accessories: one User Manual, one hanging rope.
- C. ofware description
- Release version: V2

 Please check the device and accessories according to the list to avoid that the device can not work normally.

5 Operating

- 5.1 Insert the two batteries properly to the direction, and then replace the cover.
- 5.2 Open the clip as shown in Figure 5.



Figure 5. Put finger in position

- 5.3 Let the patient's finger put into the rubber cushions of the clip (make sure the finger is in the right position), and then clip the finger.
- 5.4 Press the button once on front panel.
- 5.5 Do not shake the finger and keep the patient at ease during the process. Meanwhile, human body is not recommended in movement status.
- 5.6 Get the information directly from screen display.
- 5.7 In boot-strap state, press button, and the device is reset.
-  Fingernails and the luminescent tube should be on the same side.

6 Maintain, Transport and Storage

6.1 Cleaning and disinfection

The device must be turned off before cleaning, and it should not be immersed into liquid.

Please take out the internal battery before cleaning, do not immerse it into liquid.

Use 75% alcohol to wipe the device enclosure and the nail pad, nature dry or clean it with clean and soft cloth. Do not spray any liquid on the device directly, and avoid liquid penetrating into the device.

6.2 Maintenance

- A. Check the main unit and all accessories periodically to make sure that there is no visible damage that may affect patient's safety and monitoring performance. It is recommended that the device should be inspected weekly at least. When there is obvious damage, stop using it.
- B. Please clean and disinfect the device before/after using it according to the User Manual (6.1).
- C. Please replace the batteries in time when low-battery appears.
- D. Please take out the batteries if the device is not used for a long time.
- E. The device need not to be calibrated during maintenance.

6.3 Transport and Storage

- A. The packed device can be transported by ordinary conveyance or according to transport contract. During transportation, avoid strong shock, vibration and splashing with rain or snow, and it can not be transported mixed with toxic, harmful, corrosive material.
- B. The packed device should be stored in room with no corrosive gases and good ventilation.

7 Troubleshooting

Trouble	Possible Reason	Solution
The SpO ₂ and Pulse Rate can not be displayed normally	1) The finger is not properly inserted.	1) Please insert the finger properly and measure again.
	2) The finger is shaking or the patient is moving.	2) Let the patient keep calm.
	3) The device is not used in environment required by the manual.	3) Please use the device in normal environment.
	4) The device works abnormally.	4) Please contact the after-sales.

The SpO ₂ and Pulse Rate are not displayed stably	1) The finger is not placed inside deep enough.	1) Place the finger properly and try again.
	2) The finger is shaking or the patient is moving.	2) Let the patient keep calm
The device can not be turned on	1) The battery is drained away or almost drained away.	1) Please change batteries.
	2) The battery is assembled incorrectly.	2) Please assemble the battery again.
	3) The device's malfunction.	3) Please contact the local service center.
The display is off suddenly	1) The device enters into the energy saving mode.	1) Normal.
	2) Low battery.	2) Please charge the battery.
	3) The device works abnormally.	3) Please contact the after-sales.

8 Key of Symbols

Symbols	Meaning	Symbols	Meaning
	Follow instructions for use	PR bpm	Pulse rate (bpm)
	Type BF applied part	%SpO ₂	Pulse oxygen saturation (%)
	Manufacturer		Recyclable
	Serial number		Expiration date
	WEEE disposal	---	1. The finger clip falls off (no finger inserted) 2. Signal inadequacy indicator
	Battery anode		Battery cathode
	Covering Protection rate		Humidity limit
	Temperature limit		This way up
	Atmospheric pressure limit		Keep in a cool, dry place
	Fragile, handle with care		Alarm inhibit
	1.Exit standby mode. 2.Reset		Manufacture Date
	Lot number	P/N	Material code
	Authorized representative in the European community		Medical device
	Medical Device compliant with Regulation (EU) 2017/745		Product code
	Caution: read instructions (warnings) carefully		Imported by
	Keep away from sunlight		Unique device identifier
	The battery voltage indication is deficient (change the battery in time avoiding the inexact measure)		

Note: Your device may not contain all the following symbols.

9 Function Specification

SpO ₂ [see note 1]	
Display range	0% ~ 99%
Measured range	0% ~ 100%
Accuracy [see note 2]	
Resolution	1%
PR	
Display range	30 bpm ~ 250 bpm
Measured range	30 bpm ~ 250 bpm
Accuracy[see note 3]	
Resolution	1 bpm
Accuracy under low perfusion [see note 4]	
Light interference	

Optical sensor [see note 5]	
Red light	Wavelength: about 660 nm, optical output power:< 6.65mW
Infrared light	Wavelength: about 905 nm, optical output power:<6.75 mW
Safety class	Internally powered equipment, type BF applied part
International Protection	IP22
Working voltage	DC 2.6 V — 3.6 V
Working current	≤ 25 mA
Power supply	1.5V (AAA size) alkaline batteries × 2 or rechargeable battery
Battery life	Two batteries can work continually for 20 hours
Dimension and Weight	
Dimension	60(L) × 32.5(W) × 30.5(H) mm
Weight	About 50 g (including a lithium battery)

Note 1: the claims of SpO₂ accuracy shall be supported by clinical study measurements taken over the full range. By artificial inducing, get the stable oxygen level to the range of 70 % to 100 % SpO₂, compare the SpO₂ values collected by the secondary standard pulse oximeter equipment and the tested equipment at the same time, to form paired data, which are used for the accuracy analysis.

Note 2: because pulse oximeter equipment measurements are statistically distributed, only about two-thirds of pulse oximeter equipment measurements can be expected to fall within ±Arms of the value measured by a CO-OXIMETER.

Note 3: percentage modulation of infrared signal as the indication of pulsating signal strength, patient simulator has been used to verify its accuracy under conditions of low perfusion. SpO₂ and PR values are different due to low signal conditions, compare them with the known SpO₂ and PR values of input signal.

Note 4: optical sensors as the light-emitting components, will affect other medical devices applied the wavelength range. The information may be useful for the clinicians who carry out the optical treatment.For example, photodynamic therapy operated by clinician.

Note 5: Patient simulator has been used to verify the pulse rate accuracy, it is stated as the root-mean-square difference between the PR measurement value and the value set by simulator.

EMC

This equipment is suitable for professional healthcare facility environments and home healthcare environments

Warnings:

- Don't near active HF SURGICAL EQUIPMENT and the RF shielded room of an ME SYSTEM for magnetic resonance imaging, where the intensity of EM DISTURBANCES is high.
- Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.
- Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.
- Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the this equipment, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

Notes:

- this equipment needs special precautions regarding EMC and needs to put into service according to the EMC information provided below.
- The basic performance: SpO₂ measured range: 70% ~ 100%, absolute error: ±2%; PR measured range: 30 bpm ~ 250 bpm, accuracy: ±2 bpm or ±2%, whichever is greater.
- When the device is disturbed, the data measured may fluctuate, please measure repeatedly or in another environment to ensure its accuracy.
- Other devices may affect this device even though they meet the requirements of CISPR.

Guidance and Declaration - Electromagnetic Emissions	
Emission test	Compliance
Radiated RF emissions CISPR 11	Group 1
Radiated RF emissions CISPR 11	Class B
Harmonic distortion IEC 61000-3-2	Not applicable
Voltage fluctuations and flicker IEC 61000-3-3	Not applicable

Guidance and Declaration - Electromagnetic Immunity		
Immunity test	IEC60601 test level	Compliance level
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/	Not Applicable

	output lines	
Surge IEC 61000-4-5:	±1 kV line(s) to line(s) ±2 kV line(s) to earth	Not Applicable
Voltage dips and Voltage interruptions IEC 61000-4-11	0 % UT; 0.5 cycle At0°,45°,90°,135°,180°,225°,270°and315°; 0 % UT; 1 cycle and 70 % UT ; 25/30 cycles /Single phase:at 0°. 0 % UT ; 250/300 cycle	Not Applicable
Power frequency (50/60Hz) magnetic field IEC 61000-4-8	30 A/m 50Hz/60Hz	30 A/m 50Hz/60Hz
Conducted RF IEC61000-4-6	3 V 0.15MHz - 80 MHz 6 V in ISM and amateur radio bands between 0.15MHz to 80 MHz 80%AM at 1kHz	Not Applicable
Radiated RF IEC61000-4-3	10V/m 80 MHz-2,7GHz 80%AM at 1kHz	10V/m 80 MHz-2,7GHz 80%AM at 1kHz
OTE UT is the a.c.mains voltage prior to application of the test level		

Guidance and manufacturer's declaration - electromagnetic Immunity						
Radiated RF IEC61000-4-3 (Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment)	Test Frequency (MHz)	Band (MHz)	Service	Modulation	IEC60601 -1-2 Test level (V/m)	Compliance level (V/m)
	385	380 – 390	TETRA 400	Pulse modulation b) 18 Hz	27	27
	450	430 – 470	GMRS 460, FRS 460	FM c) ±5 kHz deviation 1 kHz sine	28	28
	710	704 – 745	LTE Band 13,17	Pulse modulation b) 217 Hz	9	9
	780	787				
	810	800 – 960	GSM 800/900, TETRA 800, IDEN 820, CDMA 850, LTE Band 5	Pulse modulation b) 18 Hz	28	28
	870					
	930	1700 – 1990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3,4,25; UMTS	Pulse modulation b) 217 Hz	28	28
	1720					
	1845					
	1970	2400 – 2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation b) 217 Hz	28	28
	2450					
	2570					
	5240	5100 – 5800	WLAN 802.11 a/n	Pulse modulation b) 217 Hz	9	9
	5500					
	5785					

 **Disposal:** The product must not be disposed of along with other domestic waste. The users must dispose of this equipment by bringing it to a specific recycling point for electric and electronic equipment

GIMA WARRANTY TERMS

The Gima 12-month standard B2B warranty applies